



[WWW.ZONERICH.COM](http://WWW.ZONERICH.COM)




**INFRARED  
THERMOMETER**

***T2020***



## FEATURES

- ❑ Ergonomically & Aesthetic Designed
- ❑ High Precision Infrared Sensor
- ❑ Quick Response & Fast Measuring
- ❑ Two Color Backlights
- ❑ Measuring Results Storage
- ❑ Beeper Alert



**MEASURE RANGE**  
25°C~100°C

**MEASURE STORAGE**  
32 DATAS

**BEEPER ALERT**

**MEASURE PRECISION**  
± 0.2°C

**BUTTON PLUS '+'**

**BUTTON SETTING**

**BUTTON MINUS '-'**

**TWO COLOR ALERT**

TEMP  
温度  
36.8°C

TEMP  
38.0°C

The image shows a purple and white infrared thermometer. The main display is green and shows a temperature of 36.8°C. Below the display are three buttons: a plus sign (+), a square (S), and a minus sign (-). A callout box on the right shows a red display with a temperature of 38.0°C, indicating a two-color alert. Various callout boxes point to specific features of the device, such as the measurement range, storage capacity, precision, and alert functions.


HIGH PRECISION  
INFRARED SENSOR

MEASURE TIME  
1 SECOND

QUICK RESPONSE  
TEST BUTTON

ERGONOMICALLY & AESTHETIC  
DESIGNS & STRUCTURE



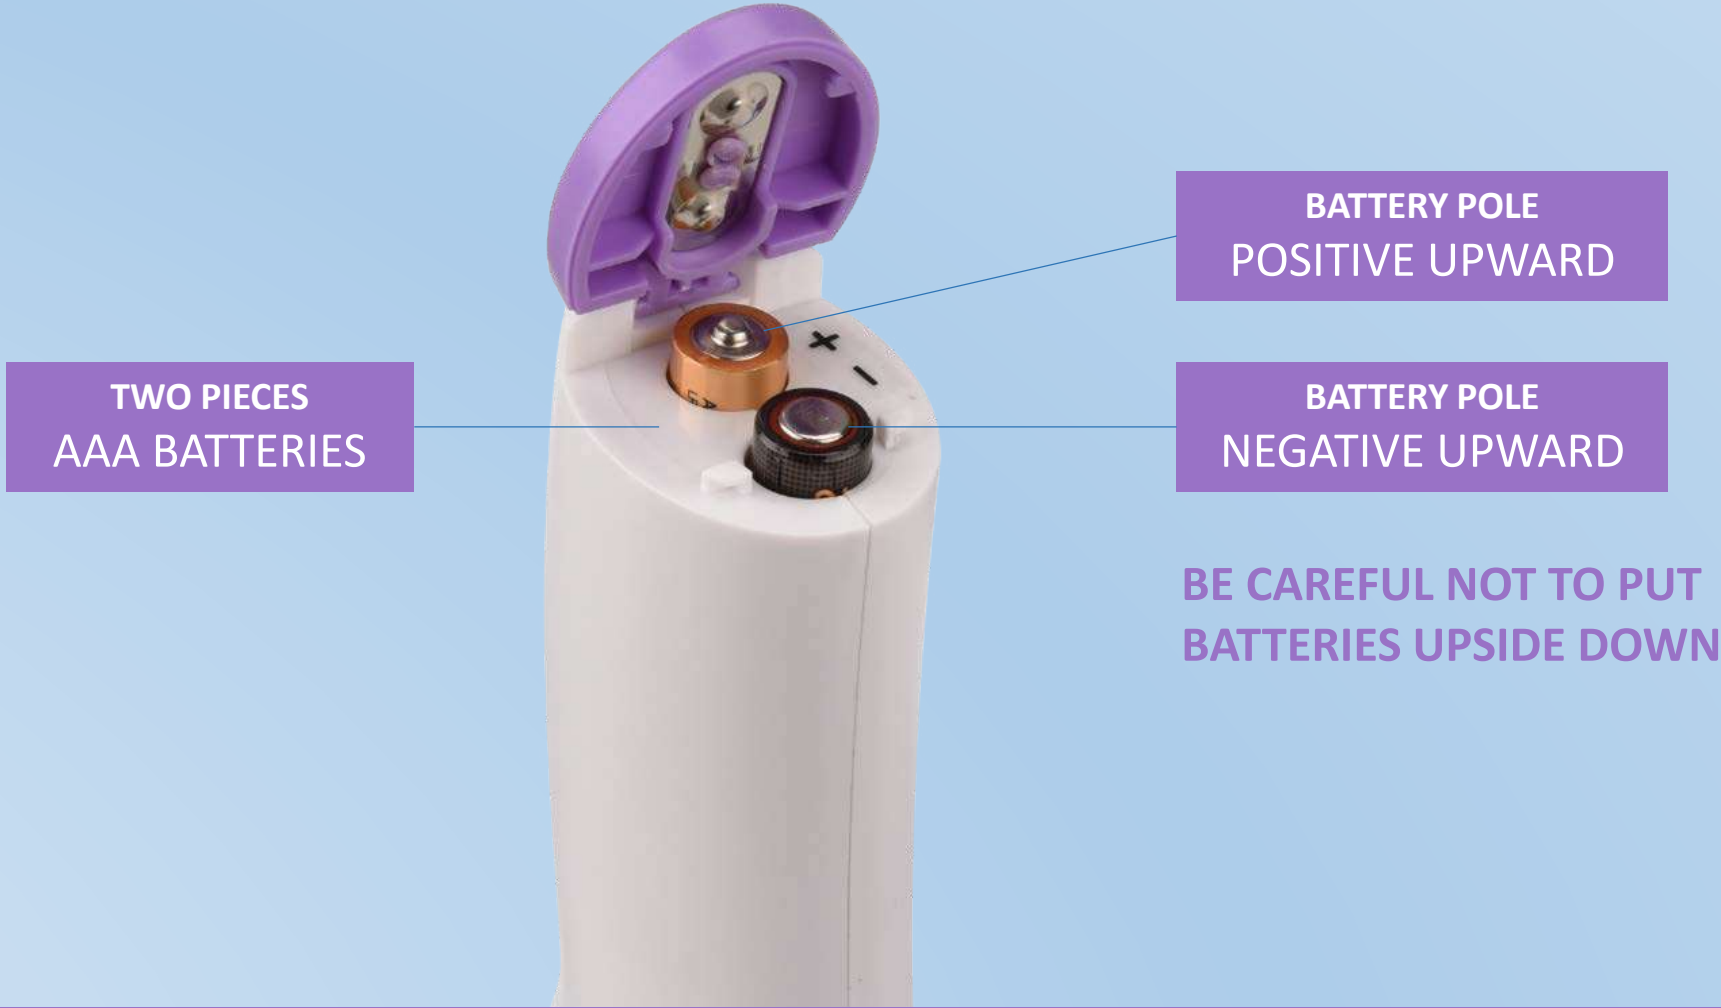


**TWO PIECES  
AAA BATTERIES**

**BATTERY POLE  
POSITIVE UPWARD**

**BATTERY POLE  
NEGATIVE UPWARD**

**BE CAREFUL NOT TO PUT  
BATTERIES UPSIDE DOWN**

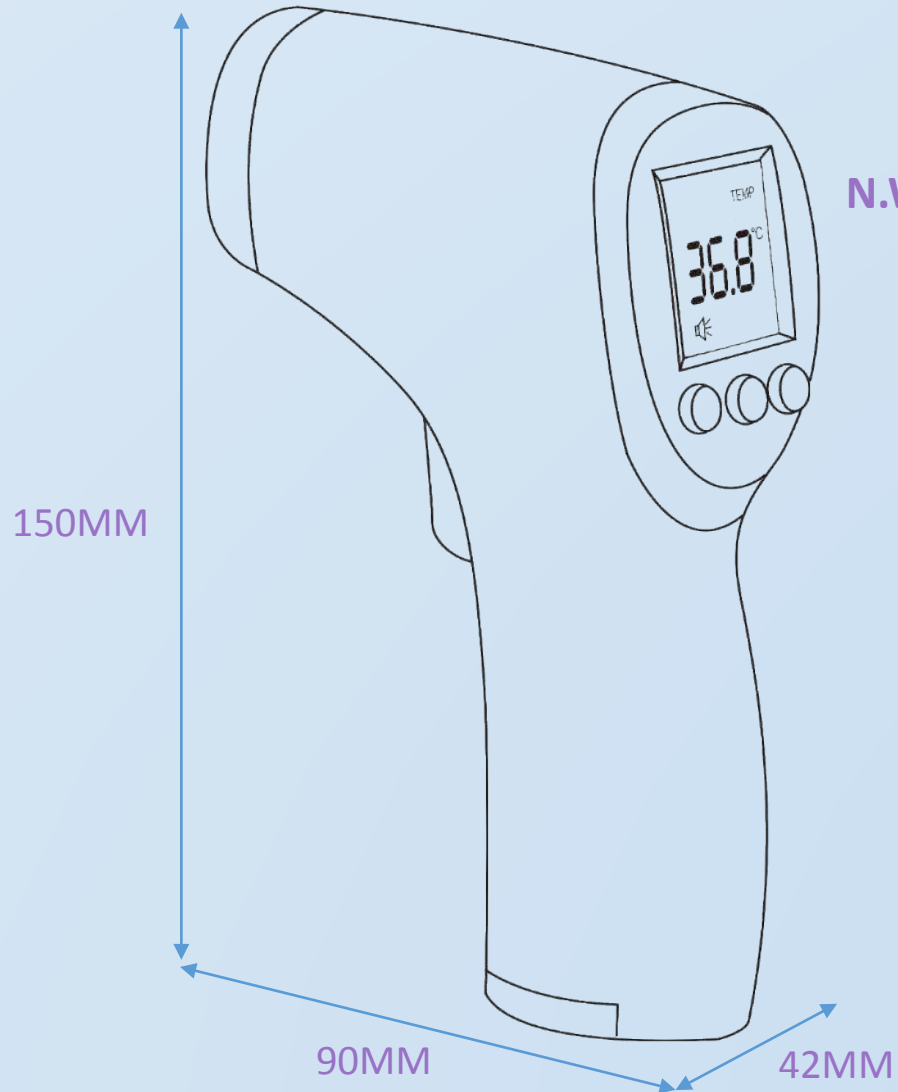

N.W.: 150G

STORAGE ENVIRONMENT  
-10°C~50°C RH≤85%

OPERATE ENVIRONMENT  
10°C~40°C RH≤85%



60PCS / CARTON  
G.W.: 11.65KG




55MM

175MM

107MM



**PACK LIST**

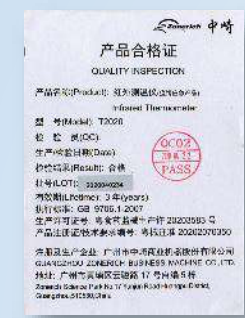




DENOMINACION TECNICA	TERMOMETRO INFRARROJO
<p>ESPECIFICACIONES TECNICAS</p> 	<p><b>Descripción del producto:</b></p> <p>Este producto mide la temperatura de la superficie de acuerdo con el principio del tamaño y la longitud de onda de la energía de radiación infrarroja liberada por el objeto.</p> <p><b>Forma de presentación:</b> Caja de cartón conteniendo 01 unidad con sus componentes y accesorios.</p> <ul style="list-style-type: none"> <li>✓ <b>Componentes:</b> Carcasa, placa de circuito, parte de medición de temperatura, pantalla, fuente de alimentación.</li> <li>✓ <b>Accesorios:</b> 02 pilas AAA, manual de usuario</li> </ul> <p><b>Especificaciones del Producto</b></p> <ul style="list-style-type: none"> <li>✓ <b>Entrada clasificada:</b> Batería DC 3V</li> <li>✓ <b>Frecuencia de funcionamiento:</b> 500 kHz</li> <li>✓ <b>Método de prueba:</b> Sin contacto</li> <li>✓ <b>Distancia de prueba:</b> 3 - 5cm</li> <li>✓ <b>Rango de modo de temperatura de superficie:</b> 25 - 100° C</li> <li>✓ <b>Rango de modo general:</b> 35 - 42° C</li> <li>✓ <b>Medida de precisión:</b> 35 - 42°C por + 0.2° C</li> <li>✓ <b>Resolución de video:</b> 0.1°C</li> <li>✓ <b>Ambiente de trabajo:</b> 10 - 40° C Humedad ≤ 85%</li> <li>✓ <b>Ambiente de almacenamiento:</b> -10 - 50° C Humedad ≤ 85%</li> <li>✓ <b>Fuente de energía:</b> DC 3V (2pcs AAA batería)</li> <li>✓ <b>Luz de fondo:</b> Verde, rojo</li> <li>✓ <b>Unidad:</b> Grados Celsius</li> <li>✓ <b>Auto deslizamiento:</b> 20 segundos</li> <li>✓ <b>Tamaños:</b> 150 x 90 x 42mm</li> <li>✓ <b>Peso:</b> 99g</li> </ul>



FORMA DE PRESENTACION	Caja de cartón conteniendo 01 unidad con sus componentes y accesorios.
NOMBRE DEL DISPOSITIVO MEDICO	INFRARED THERMOMETER (TERMOMETRO INFRARROJO)
MODELO	AT600, T2020
REGISTRO SANITARIO	EN TRAMITE DE INSCRIPCION



INDICAR IMPORTADO o NACIONAL	IMPORTADO
FABRICANTE	GUANGZHOU ZONERICH BUSINESS MACHINE CO. LTD.
PAIS	CHINA

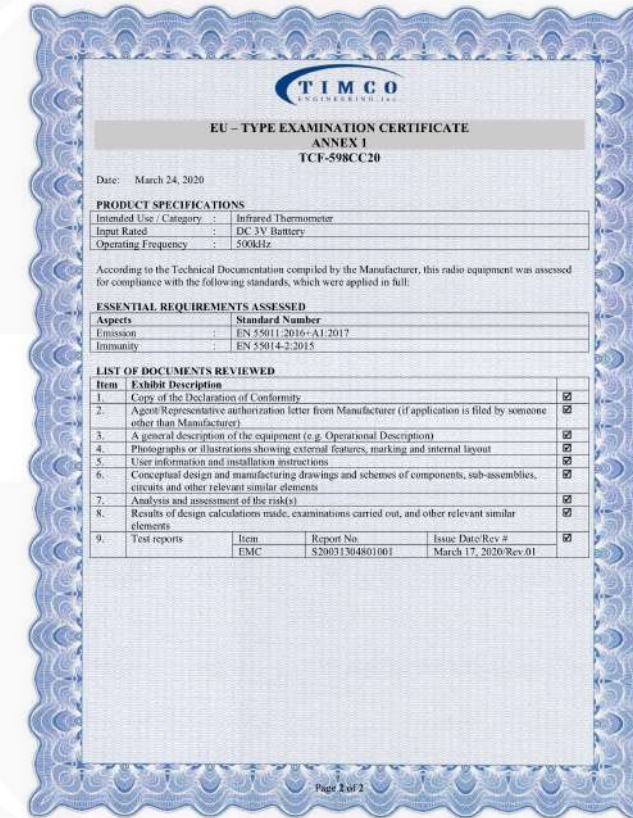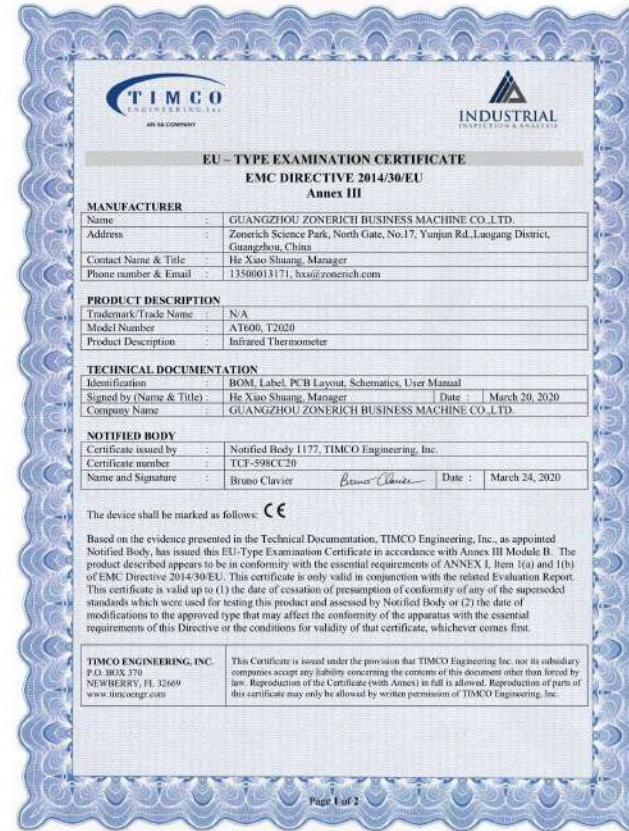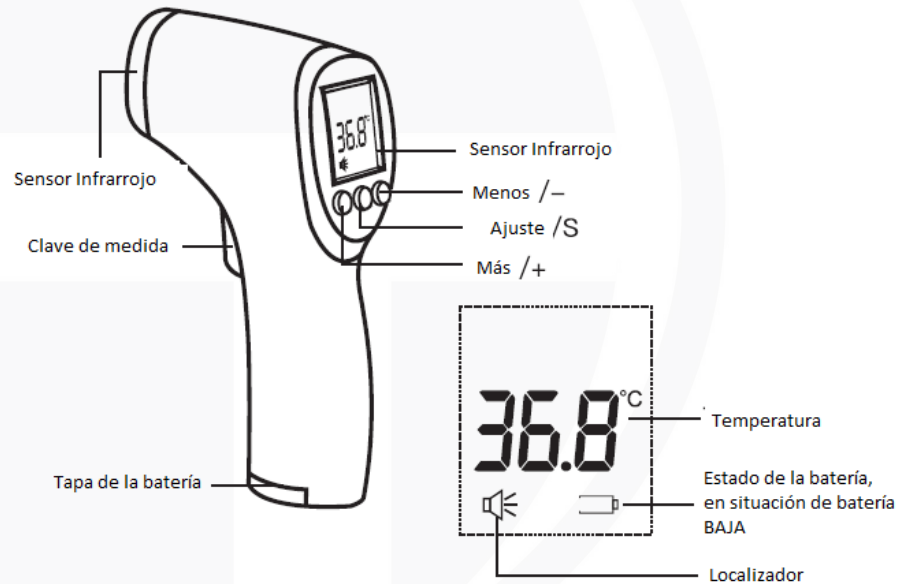



**CERTIFICATE OF CONFORMITY OF QUALITY  
MANAGEMENT SYSTEM CERTIFICATION**  
NO: 08919Q20423R5M

This Is To Certify That The Quality Management System Of  
**GUANGZHOU ZONERICH BUSINESS MACHINE CO.,LTD**  
North Gatd, No.17 YunJun RD., LuoGang District, GuangZhou City,  
Guangdong, P.R. China  
Unified Social Credit Code: 9144010174991105X7 Post Code: 510530

Quality Management System Complies With:  
**GB/T19001-2016/ISO9001:2015 Standard**

Scope:  
R&D, Manufacture And Service Of Printer, Cash Register(Approved By CCC)

Date of issue: 2019-3-19 Expiry date: 2022-3-18  
Holding this certificate organizations receive annual surveillance audits qualified, And administrative license valid state regulations

Approval of the first surveillance audit Zhongshui Brilliant Certification Co., Ltd.	Approval of the second surveillance audit Zhongshui Brilliant Certification Co., Ltd.	Approval of the third surveillance audit Zhongshui Brilliant Certification Co., Ltd.
---	--	---





中国认可  
国际互认  
管理体系  
MANAGEMENT SYSTEM  
CNAS C089-M

Representative of The Company  
The Certificate Information Can Be Inquired At <http://www.cnca.gov.cn> Or <http://www.zsbc.net>  
Tel:010-82272603 Add:Room 7001-7004 Block B Tiancheng Technology Building Of No.2 Xinfeng Street Desai Avenue Xichang District Beijing



**质量管理体系认证证书**  
编号: 08919Q20423R5M  
兹 证 明

**广州市中崎商业机器股份有限公司**  
广东省广州市萝岗区云骏路 17 号自编 5 栋  
统一社会信用代码: 9144010174991105X7 邮编: 510530

其质量管理体系符合:  
**GB/T19001-2016/ISO9001:2015 标准**

认证范围:  
打印机、收款机的研发、生产与服务 (CCC 许可范围内)

颁证日期: 2019 年 3 月 19 日 有效期至: 2022 年 3 月 18 日  
持本证书组织接受年度监督审核合格, 并在国家规定的行政许可有效期内使用有效

第一次监督合格标志 (贴花)	第二次监督合格标志 (贴花)	第三次监督合格标志 (贴花)
-------------------	-------------------	-------------------





中国认可  
国际互认  
管理体系  
MANAGEMENT SYSTEM  
CNAS C089-M

公司代表 (签名)  
本证书信息可在北京中水卓越认证有限公司官方网站 (<http://zsbc.net>) 及国家认证认可监督管理委员会官方网站 (<http://www.cnca.gov.cn>) 上查询, 电话: 010-82272603 地址: 北京市西城区德胜大街新凤街 2 号天成科技大厦 B 座 7001-7004